

The validation of simplified EEG derived from the bispectral index monitor in post-cardiac arrest patients.

Peer-reviewed author version

Haesen, Jolien; EERTMANS, Ward; GENBRUGGE, Cornelia; MEEEX, Ingrid; Demeestere, Jelle; VANDER LAENEN, Margot; BOER, Willem; MESOTTEN, Dieter; DENS, Jo; JANS, Frank; Ernon, Ludovic & DE DEYNE, Cathy (2018) The validation of simplified EEG derived from the bispectral index monitor in post-cardiac arrest patients.. In: RESUSCITATION, 126, p. 179-184.


DOI: 10.1016/j.resuscitation.2018.01.042

Handle: <http://hdl.handle.net/1942/25876>

## Accepted Manuscript

Title: The validation of simplified EEG derived from the bispectral index monitor in post-cardiac arrest patients

Authors: Jolien Haesen, Ward Eertmans, Cornelia Genbrugge, Ingrid Meex, Jelle Demeestere, Margot Vander Laenen, Willem Boer, Dieter Mesotten, Jo Dens, Frank Jans, Ludovic Ernon, Cathy De Deyne

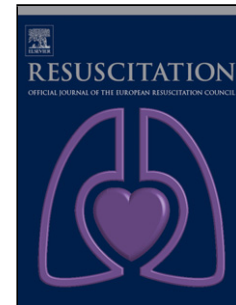

PII: S0300-9572(18)30052-2  
DOI: <https://doi.org/10.1016/j.resuscitation.2018.01.042>  
Reference: RESUS 7473

To appear in: *Resuscitation*

Received date: 28-10-2017  
Revised date: 11-1-2018  
Accepted date: 27-1-2018

Please cite this article as: Haesen Jolien, Eertmans Ward, Genbrugge Cornelia, Meex Ingrid, Demeestere Jelle, Laenen Margot Vander, Boer Willem, Mesotten Dieter, Dens Jo, Jans Frank, Ernon Ludovic, De Deyne Cathy. The validation of simplified EEG derived from the bispectral index monitor in post-cardiac arrest patients. *Resuscitation* <https://doi.org/10.1016/j.resuscitation.2018.01.042>

This is a PDF file of an unedited manuscript that has been accepted for publication. As a service to our customers we are providing this early version of the manuscript. The manuscript will undergo copyediting, typesetting, and review of the resulting proof before it is published in its final form. Please note that during the production process errors may be discovered which could affect the content, and all legal disclaimers that apply to the journal pertain.

# The validation of simplified EEG derived from the bispectral index monitor in post-cardiac arrest patients

Jolien Haesen, MSc

Department of Medicine and Life Sciences, Hasselt University, Diepenbeek, Belgium

Department of Anaesthesiology, Intensive Care, Emergency Medicine and Pain Therapy,

Ziekenhuis Oost-Limburg, Genk, Belgium

Schiepse Bos 6, 3600 Genk, Belgium

[haesenjolien2@hotmail.com](mailto:haesenjolien2@hotmail.com)

Ward Eertmans, MSc (*Contributed equally*)

Department of Medicine and Life Sciences, Hasselt University, Diepenbeek, Belgium

Department of Anaesthesiology, Intensive Care, Emergency Medicine and Pain Therapy,

Ziekenhuis Oost-Limburg, Genk, Belgium

Schiepse Bos 6, 3600 Genk, Belgium

[ward.eertmans@uhasselt.be](mailto:ward.eertmans@uhasselt.be)

Cornelia Genbrugge, MD, PhD

Department of Medicine and Life Sciences, Hasselt University, Diepenbeek, Belgium

Department of Anaesthesiology, Intensive Care, Emergency Medicine and Pain Therapy,

Ziekenhuis Oost-Limburg, Genk, Belgium

Schiepse Bos 6, 3600 Genk, Belgium

[cornelia.genbrugge@uhasselt.be](mailto:cornelia.genbrugge@uhasselt.be)

Ingrid Meex, MSc, PhD

Department of Medicine and Life Sciences, Hasselt University, Diepenbeek, Belgium

Department of Anaesthesiology, Intensive Care, Emergency Medicine and Pain Therapy,

Ziekenhuis Oost-Limburg, Genk, Belgium

Schiepse Bos 6, 3600 Genk, Belgium

[ingrid.meex@zol.be](mailto:ingrid.meex@zol.be)

Jelle Demeestere, MD

Department of Neurology, University Hospitals Leuven, Belgium

Herestraat 49, 3600 Leuven, Belgium [jelle.demeestere@kuleuven.be](mailto:jelle.demeestere@kuleuven.be)

Margot Vander Laenen, MD

Department of Anaesthesiology, Intensive Care, Emergency Medicine and Pain Therapy,

Ziekenhuis Oost-Limburg, Genk, Belgium

Schiepse Bos 6, 3600 Genk, Belgium

[margot.vanderlaenen@zol.be](mailto:margot.vanderlaenen@zol.be)

Willem Boer, MD

Department of Anaesthesiology, Intensive Care, Emergency Medicine and Pain Therapy,

Ziekenhuis Oost-Limburg, Genk, Belgium

Schiepse Bos 6, 3600 Genk, Belgium

[willem.boer@zol.be](mailto:willem.boer@zol.be)

Dieter Mesotten, MD, PhD

Department of Medicine and Life Sciences, Hasselt University, Diepenbeek, Belgium

Department of Anaesthesiology, Intensive Care, Emergency Medicine and Pain Therapy,

Ziekenhuis Oost-Limburg, Genk, Belgium

Schiepse Bos 6, 3600 Genk, Belgium

[dieter.mesotten@zol.be](mailto:dieter.mesotten@zol.be)

Jo Dens, MD, PhD

Department of Medicine and Life Sciences, Hasselt University, Diepenbeek, Belgium

Department of Cardiology, Ziekenhuis Oost-Limburg, Genk, Belgium

Schiepse Bos 6, 3600 Genk, Belgium

[jo.dens@zol.be](mailto:jo.dens@zol.be)

Frank Jans , MD, PhD

Department of Medicine and Life Sciences, Hasselt University, Diepenbeek, Belgium

Department of Anaesthesiology, Intensive Care, Emergency Medicine and Pain Therapy,

Ziekenhuis Oost-Limburg, Genk, Belgium

Schiepse Bos 6, 3600 Genk, Belgium

[frank.jans@zol.be](mailto:frank.jans@zol.be)

Ludovic Ernon, MD

Department of Neurology, Ziekenhuis Oost-Limburg, Genk, Belgium

Schiepse Bos 6, 3600 Genk, Belgium

[ludovic.ernon@zol.be](mailto:ludovic.ernon@zol.be)

Cathy De Deyne, MD, PhD

Department of Medicine and Life Sciences, Hasselt University, Diepenbeek, Belgium

Department of Anaesthesiology, Intensive Care, Emergency Medicine and Pain Therapy,

Ziekenhuis Oost-Limburg, Genk, Belgium

Schiepse Bos 6, 3600 Genk, Belgium

[cathy.dedeyne@zol.be](mailto:cathy.dedeyne@zol.be)

# **Total word count**

Paper = 2936 words

Abstract = 250 words

**Corresponding author**

Eertmans Ward

[ward.eertmans@uhasselt.be](mailto:ward.eertmans@uhasselt.be)

Tel: 0032 89 32 15 14

Fax: 0032 89 32 79 00

ACCEPTED MANUSCRIPT

## **Abstract**

### **Aims**

We aimed to validate retrospectively the accuracy of simplified electroencephalography (EEG) monitoring derived from the bispectral index (BIS) monitor in post-cardiac arrest (CA) patients.

### **Methods**

Successfully resuscitated CA patients were transferred to the Catheterization Lab followed by percutaneous coronary intervention when indicated. On arrival at the coronary care unit, bilateral BIS monitoring was started and continued up to 72 hours. Raw simplified EEG tracings were extracted from the BIS monitor at a time point coinciding with the registration of standard EEG monitoring. BIS EEG tracings were reviewed by two neurophysiologists, who were asked to indicate the presence of following patterns: diffuse slowing rhythm, burst suppression pattern, cerebral inactivity, periodic epileptiform discharges and status epilepticus (SE). Additionally, these simplified BIS EEG tracings were analysed by two inexperienced investigators, who were asked to indicate the presence of SE only.

### **Results**

Thirty-two simplified BIS EEG samples were analysed. Compared to standard EEG, neurophysiologists interpreted all simplified EEG samples with a sensitivity of 86%, a specificity of 100% and an interobserver variability of 0.843. Furthermore, SE was identified with a sensitivity of 80% and a specificity of 94% by two inexperienced physicians.

### **Conclusion**

Using a simple classification system, raw simplified EEG derived from a BIS monitoring device is comparable to standard EEG monitoring. Moreover, investigators without EEG experience were capable to identify SE in post-CA patients. Future studies will be warranted to confirm our results and to determine the added value of using simplified BIS EEG in terms of prognostic and therapeutic implications.

**Key words**

Bispectral index – simplified electroencephalography – neuromonitoring – cardiac arrest – status epilepticus



## Introduction

Up to one third of the cardiac arrest (CA) survivors develop seizures which often remain underdiagnosed as most of them are classified as non-convulsive ones.<sup>1, 2</sup> Multiple studies already showed that the development of seizures is associated with a poor prognosis.<sup>3, 4</sup> Moreover, early detection of these seizures is of the utmost importance since mortality increases exponentially with their duration.<sup>2, 5, 6</sup> Unfortunately, there is still a delay in the identification of these harmful seizures in most post-CA patients as full or continuous EEG (cEEG) recording is rarely performed in the early hours following CA.<sup>7, 8</sup> This emphasizes the need for a simple but accurate EEG tool to identify aggravating neurological conditions and secondary cerebral insults such as epileptic activity. Patients who experience epileptic seizures might benefit the most from a specific treatment in case of early detection.<sup>9-12</sup>

The bispectral index (BIS) monitor is an easy to use and rapidly deployable 4-channel quantitative EEG system.<sup>13</sup> Although the BIS monitor, with incorporated BIS value calculation (0 – 100), is developed to measure the depth of consciousness during general anaesthesia, several studies have used the BIS value to guide neurological prognostication after CA.<sup>14, 15</sup> The overall goal of this study, however, was to validate retrospectively simplified raw EEG tracings derived from the BIS monitor against standard EEG monitoring in order to identify seizures and other ominous patterns often observed in post-CA patients.

## Methods

From March 2011 to April 2014, all adult comatose patients successfully resuscitated CA patients were admitted to the coronary care unit (CCU) in Ziekenhuis Oost-Limburg (Genk, Belgium). This retrospective study, based on prospectively gathered BIS data, aimed to validate the accuracy of simplified EEG obtained from the BIS monitor (BIS EEG) against full intermittent EEG. Therefore, only patients in whom the BIS monitor was still applied at the moment a full intermittent EEG was performed, were retrospectively selected for enrolment in this validation study. Approval of the local ethical committee was obtained before the onset of the study (CME11/066) and written informed consent was obtained from the patient's next of kin and was reconfirmed if patients regained consciousness.

### Patient management

According to the institutional protocol, targeted temperature management (TTM) at 33°C was immediately started after admission to the emergency department and was further maintained at the CCU for 24 hours after which patients were gradually rewarmed at a rate of 0.3°C/h over the following 12 hours.<sup>16, 17</sup> Sedation was maintained by intravenous administration of propofol, midazolam and remifentanyl. In line with current guidelines, patients received cisatracurium only in case of shivering. All patients were intubated and mechanically ventilated. At the end of rewarming, sedation was reduced to facilitate assessment of patients' neurological status. Patients unready for extubation due to respiratory, circulatory complications or due to persisting coma remained sedated with the lowest dose necessary to tolerate endotracheal intubation. Full standard EEG registrations were performed routinely after the return to normothermia (i.e. at about 36 hours after CA) or in case of a clinical indication. These EEG measurements were digitally recorded with a 19-channel system, arranged according to the international 10-20 system. Every EEG was characterized by a description of the posterior dominant rhythm (or absence thereof) and amplitude as well as the presence of non-dominant rhythms. Lateralization and the presence of artefacts was described where applicable. If present, epileptic activity was described as interictal, ictal or as status

epilepticus. Patients with epileptic activity, based on standard EEG measurements, were treated with antiepileptic drugs, often in combination with midazolam and propofol. Although treating physicians were not blinded, BIS values were not used for titrating depth of sedation. Furthermore, withdrawal of life support was not based on the simplified EEG measurements displayed on the BIS monitor, but was in line with international guidelines and relied on a clinical evaluation, full EEG measurements and somatosensory evoked potentials (SSEP) instead.<sup>18</sup>

### **Bispectral index monitoring**

On arrival at the CCU, bilateral BIS monitoring using the BIS VISTA™ (Aspect Medical Systems, Inc. Norwood, USA) was started as soon as possible and continued up to 72 hours. The BIS monitor provides a real-time number using an easily applicable six-electrode forehead sensor (BIS™ bilateral sensor), which was applied to the frontotemporal area before the start of TTM. Aside from the BIS value itself, the BIS VISTA™ monitor also displays bilateral frontotemporal EEG traces (Fig. 1). To compare these simplified EEG traces derived from the BIS monitor with standard intermittent EEG, raw BIS EEG traces of at least five consecutive minutes were retrospectively extracted at a time point that coincided with the registration of a standard full EEG using the DATALOGGER Data Review Program for Windows (Aspect Medical Systems inc.;version 0.04.07;1995). Afterwards, these small BIS EEG frames were reviewed by two experienced neurophysiologists (LE and JD) who were blinded to patients' clinical course and neurological outcome. They were asked to indicate the presence of five simple EEG patterns (i.e. diffuse slowing rhythm, burst suppression pattern, cerebral inactivity, epileptic activity/PEDs or status epilepticus (SE)) based on the classification system used by Rundgren et al.<sup>19, 20</sup> After calculating the inter-observer variability, a consensus decision was made by the two neurophysiologists in case of any discrepancies.

In order to further validate the ease of use of the simplified BIS EEG by unexperienced physicians, two investigators (IM and CG) without any experience in the interpretation of EEG, analysed the same simplified BIS EEG frames as were given to the neurophysiologists. They were specifically asked to focus only on the detection of epileptiform activity. Figure 2 was used as an

example of typical EEG tracings after CA in order to instruct the non-qualified investigators.

### **Data collection**

Baseline demographics including gender, age and information regarding drug administration were extracted from the electronic medical record. Cardiopulmonary resuscitation (CPR) details such as initial rhythm and bystander CPR were extracted from the Utstein data. Time to return to spontaneous circulation (ROSC) was determined as time of collapse to time of ROSC. Patients' outcome was graded according to the Cerebral Performance Category (CPC) score at 6 months.<sup>21</sup> CPC-scores were dichotomized as good (CPC 1-2) or poor neurological outcome (CPC 3-5).

### **Statistical analysis**

All analyses were conducted using SPSS Version 24.0 (IBM Corp., Armonk, NY, USA). Continuous data were presented as mean with standard deviation and categorical variables as counts and percentages (%). Equal distribution was tested using a Shapiro-Wilk test. Depending on normality, categorical data were analysed using a Fisher exact or a Pearson Chi-Square test, while an unpaired T-test or Mann-Whitney U test was used for continuous data. Correlations were calculated using Pearson's or Spearman's coefficient of correlation, depending on normality. Sensitivity and specificity were calculated for the correct detection of the aforementioned five EEG patterns. A p-value < 0.05 was considered significant.

## Results

### Patient characteristics

Between 2011 and 2014, 115 comatose CA survivors were enrolled in this study and BIS monitoring was started in 88 patients treated with TTM at 33°C (Fig. 3). Thirteen subjects were excluded due to invalid data caused by technical difficulties ( $n = 12$ ) and hemodynamic instability resulting in death within the initial hours following admission ( $n = 1$ ). In 32 out of these 75 retained patients, the BIS monitor was still applied at a time point coinciding with the performance of a full standard EEG. At 180 days post-CA, 14 out of these 32 patients (44%) had a good neurological outcome (CPC1-2), while 18 patients (56%) had a CPC of 5. There were no patients with a CPC of 3 or 4 at 180 days post-CA. Baseline characteristics of both outcome groups are summarized in table 1. Interestingly, all patients who experienced a SE had a poor neurological outcome ( $p < 0.001$ ).

### Validation

In total, 32 simplified BIS EEG samples were analysed at a time point coincident with the registration of full standard EEG monitoring, in order to compare the concordance of both EEG options. The time of validation was at day  $3 \pm 1$  after CA and was not different between patients with a good and poor neurological outcome ( $p = 0.613$ ; Table 1). According to the standard EEG measurements, 11 (34%) recordings showed a diffuse slowing pattern, six (19%) a burst suppression pattern, three (9%) recordings showed cerebral inactivity, four (13%) indicated PEDs and 8 (25%) recordings showed a SE (Table 2). As compared to these standard EEG measurements, neurophysiologist I misinterpreted simplified BIS EEG samples, whereas neurophysiologist II misdiagnosed six of them. As such, neurophysiologist I classified all analysed BIS EEG samples with a sensitivity of 86% and a specificity of 91%, while neurophysiologist II reached a sensitivity and specificity of 71% and 100%, respectively. After consensus was actively asked for, all BIS EEG samples were correctly analysed with a sensitivity of 86% and a specificity of 100% (Table 2).

In fact, only one SE was missed by one neurophysiologist. Most other misdiagnosed recordings showed a pattern of PEDs according to the standard EEG measurements, while the

simplified BIS EEG samples were interpreted as a diffuse slowing pattern. Three of them (75%) were misinterpreted by both neurophysiologists. Therefore, sensitivity for the classification of PEDs based on simplified BIS EEG samples is 25%.

A high level of agreement was observed between the two independent neurophysiologists ( $\kappa = 0.843$ ). There was a strong correlation between full and simplified BIS EEG for both neurophysiologists, with a mean correlation of  $r = 0.810$  ( $r_{\text{neurophysiologist I}} = 0.852$  and  $r_{\text{neurophysiologist II}} = 0.767$ ).

To test whether physicians without any EEG experience would be able to detect epileptic activity using simplified BIS EEG traces, two independent and unexperienced investigators were asked to indicate the presence of a SE on the same BIS EEG samples as were given to the neurophysiologists. One investigator missed only one patient diagnosed with SE, whereas the other investigator missed three patients. Additionally, three patients without SE on full EEG were falsely indicated as at risk for epileptic activity. As such, one investigator identified patients diagnosed with SE with a sensitivity of 90% and a specificity of 92%, whereas the other one reached a sensitivity of 70% and a specificity of 96%.

## Discussion

This was a retrospective validation study showing that: 1) raw simplified EEG traces derived from a BIS monitor correlate well with standard EEG when a simple classification system is being used in a post-CA-setting, and 2) non-experienced investigators are able to detect epileptic activity/SE on the BIS EEG monitor with a high level of accuracy.

To date, it remains to be elucidated whether the treatment of seizures effectively improves neurological outcome, or that seizures are simply a clinical expression of the post-ischemic damage questioning the benefit of any treatment efforts. Nonetheless, guidelines still advocate the use of anti-convulsive therapy in case of seizures, and therefore cEEG monitoring has been recommended in comatose CA patients treated with TTM.<sup>18, 22</sup> Unfortunately, cEEG is expensive and labour-intensive but more importantly, most of the available cEEG devices still require continuous availability of expertise for a correct interpretation. In order to become generally applicable, it should be simple, cost-effective and easy to use at the bedside.<sup>23-25</sup> A simplified EEG monitor would overcome these limitations and would allow us at the same time to detect non-convulsive seizures in an early stage.

Numerous studies have already investigated BIS monitoring to assist in neurological prognostication after CA.<sup>14, 15, 26</sup> Furthermore, it has been suggested that the BIS monitor might be used to detect non-convulsive seizures as their occurrence is accompanied with fluctuations of the BIS value.<sup>27-30</sup> In fact, the BIS monitor samples raw EEG tracings to provide the real-time BIS value. Although these raw EEG tracings are displayed in real-time, the potential to use the BIS device as a simplified EEG monitor after OHCA has not been investigated.

Rundgren et al. already investigated in OHCA patients the prognostic role of amplitude-integrated EEG, another simplified EEG tool, although it was not fully validated against standard EEG.<sup>19, 20</sup> It is for this reason that we preferred to validate first the accuracy of simplified EEG traces obtained by the BIS monitor before providing prognostic values. As such, a similar classification system, as suggested by Rundgren et al., was used consisting out of five simple EEG patterns, i.e. diffuse slowing, burst suppression, cerebral inactivity, PEDs and SE. Using this simple classification

system, this study showed a high concordance between standard and simplified BIS EEG monitoring ( $r = 0.810$ ). While other studies were able to detect a SE with a sensitivity ranging from 60% to 100%, this study reached an overall sensitivity of 86%, not only for the diagnosis of SE, but for the detection of the entire classification system.<sup>31-34</sup> This strongly indicates that simplified BIS EEG monitoring could be used to detect other ominous EEG patterns aside from a SE as well. In fact, only 9% of all BIS EEG samples were misdiagnosed by both neurophysiologists, all from patients diagnosed with PEDs. It is plausible to assume that these promising results can be partially explained by the combined use of a simplified classification system and simplified EEG monitoring device. Still, early detection of pathologic EEG tracings using a simplified EEG device can only be relevant if it either influences the course of the disease beneficially or if it would assist with the process of neuroprognostication. In this context, our data should be considered as hypothesis-generating since our study results only show that simplified BIS EEG correlate well with standard EEG. Future studies will now be warranted to validate our results and to determine the added value of using simplified BIS EEG in terms of prognostic and therapeutic implications. Unfortunately, our time point of validation was situated approximately three days after CA. As previous studies showed that the prognostic power of EEG lies within the first 24 hours, we acknowledge that the prognostic value of simplified BIS EEG warrants further examination in a similar time window<sup>14, 15, 35-37</sup>.

Aside from experienced neurophysiologists, treating physicians should also be capable of interpreting simplified EEG traces on the BIS monitor as they can play a prominent role in the early identification of epileptic activity. This study showed that even unexperienced investigators were able to indicate the presence of a SE with an adequate sensitivity (mean 80%) and specificity (mean 94%). Three patients, however, were identified as at risk for epileptic activity, although no epileptic activity was present on full EEG. Nevertheless, we believe that in case of uncertainty, it is more important to consider treatment for epileptic activity and/or request full EEG measurements as soon as possible rather than delaying until the patient is undoubtedly diagnosed with SE. Although the



benefit of anti-convulsive therapy remains indistinct, this study confirms that electrographic seizures are associated with poor neurological outcome.

In line with our study findings, others already demonstrated the ability of diverse simplified EEG systems with three to seven channels to detect epilepsy accurately.<sup>31, 33</sup> In contrast, Kolls et al. did not confirm the high compliance between a full and simplified hairline EEG system, as only 71% of the samples were correctly interpreted.<sup>32</sup> However, the EEGs samples analysed by Kolls et al. consisted out of very specific EEG patterns (e.g. GPEDs, PLEDs), which are far more difficult to diagnose as compared to the more prominent EEG patterns in post-CA patients. Similarly, we tested the accuracy of our simplified BIS EEG tool to detect PEDs and found that the sensitivity for the detection of these specific patterns was only 25%. This could be explained by the fact that these PEDs as well as other focal epileptic discharges might occur outside the frontotemporal range detected by our simplified BIS EEG device. Therefore, we believe that a simplified EEG monitoring tool should preferably be used to screen for generalized ominous patterns such as cerebral inactivity or SE instead of using it to detect very specific EEG patterns<sup>14, 15, 38</sup>. However, it has to be stated that a full EEG will always be necessary to confirm the diagnosis based on simplified BIS EEG.

### **Limitations**

Several limitations should be acknowledged. First, this validation study was a retrospective analysis which is inherently susceptible to limitations such as selection bias and missing data.. In addition, a single-centre study could have biased the visual analysis of the EEG findings. Therefore, we asked two independent neurophysiologists blinded to each other's results although it has to be stated that a third neurophysiologist to reach consensus would eliminate the risk of a self-fulfilling prophecy. Nevertheless, this validation study should be considered as a hypothesis-generating one which requires confirmation in future multicentre studies with a larger sample size. Secondly, treating physicians were not blinded to the EEG tracings displayed on the BIS monitor as visual confirmation was needed to assure adequate signal quality. Nevertheless, the recorded BIS EEG tracings were not considered for the withdrawal of treatment policy. Finally, the BIS monitor

comprises only the frontotemporal area, which does not provide information about other parts of the brain. Nonetheless, CA generally induces global ischemic brain damage, possibly implying that a frontotemporal sensor might be sufficient to provide valuable electrographic information, especially in the early hours following OHCA where there is often hardly any neuromonitoring present.

## Conclusion

This retrospective analysis shows that raw simplified EEG derived from a BIS monitoring device might be comparable to standard EEG monitoring when a simple classification system is being used by experienced neurophysiologists. Furthermore, investigators without any EEG experience were also able to identify epileptic activity in post-CA patients with an adequate accuracy. Nevertheless, multicenter studies are warranted to verify our preliminary study findings and should consider validation sessions at time points where EEG encompasses the highest prognostic power. Additionally, these studies should also determine whether BIS EEG monitoring could influence neurological outcome by detecting epileptic activity in an early phase followed by immediate anti-convulsive therapy.

**Conflicts of interests**

The authors declare that they have no competing interests.

ACCEPTED MANUSCRIPT

**Acknowledgements**

The authors wish to thank the nursing and medical staff of the emergency department, the catheterization lab, the CCU and the department of neurology for their cooperation in this study.

This study was part of the Limburg Clinical Research Program supported by the foundation Limburg Sterk Merk, Hasselt University, Ziekenhuis Oost – Limburg and Jessa Hospital.

ACCEPTED MANUSCRIPT

## References

1. Claassen J, Mayer SA, Kowalski RG, Emerson RG, Hirsch LJ. Detection of electrographic seizures with continuous EEG monitoring in critically ill patients. *Neurology*. 2004;62(10):1743-8.
2. Knight WA, Hart KW, Adeoye OM, Bonomo JB, Keegan SP, Ficker DM, et al. The incidence of seizures in patients undergoing therapeutic hypothermia after resuscitation from cardiac arrest. *Epilepsy Res*. 2013;106(3):396-402.
3. Legriel S, Hilly-Ginoux J, Resche-Rigon M, Merceron S, Pinoteau J, Henry-Lagarrigue M, et al. Prognostic value of electrographic postanoxic status epilepticus in comatose cardiac-arrest survivors in the therapeutic hypothermia era. *Resuscitation*. 2013;84(3):343-50.
4. Lybeck A, Friberg H, Aneman A, Hassager C, Horn J, Kjaergaard J, et al. Prognostic significance of clinical seizures after cardiac arrest and target temperature management. *Resuscitation*. 2017;114:146-51.
5. Legriel S, Bruneel F, Sediri H, Hilly J, Abbosh N, Lagarrigue MH, et al. Early EEG monitoring for detecting postanoxic status epilepticus during therapeutic hypothermia: a pilot study. *Neurocrit Care*. 2009;11(3):338-44.
6. Towne AR, Pellock JM, Ko D, DeLorenzo RJ. Determinants of mortality in status epilepticus. *Epilepsia*. 1994;35(1):27-34.

7. Rittenberger JC, Popescu A, Brenner RP, Guyette FX, Callaway CW. Frequency and timing of nonconvulsive status epilepticus in comatose post-cardiac arrest subjects treated with hypothermia. *Neurocrit Care*. 2012;16(1):114-22.
8. Mani R, Schmitt SE, Mazer M, Putt ME, Gaieski DF. The frequency and timing of epileptiform activity on continuous electroencephalogram in comatose post-cardiac arrest syndrome patients treated with therapeutic hypothermia. *Resuscitation*. 2012;83(7):840-7.
9. Hirsch LJ, Claassen J. The current state of treatment of status epilepticus. *Curr Neurol Neurosci Rep*. 2002;2(4):345-56.
10. Fujikawa DG. Prolonged seizures and cellular injury: understanding the connection. *Epilepsy Behav*. 2005;7 Suppl 3:S3-11.
11. Ruijter BJ, van Putten MJ, Horn J, Blans MJ, Beishuizen A, van Rootselaar AF, et al. Treatment of electroencephalographic status epilepticus after cardiopulmonary resuscitation (TELSTAR): study protocol for a randomized controlled trial. *Trials*. 2014;15:433.
12. Rossetti AO, Oddo M, Liaudet L, Kaplan PW. Predictors of awakening from postanoxic status epilepticus after therapeutic hypothermia. *Neurology*. 2009;72(8):744-9.
13. Johansen JW. Update on bispectral index monitoring. *Best Pract Res Clin Anaesthesiol*. 2006;20(1):81-99.

14. Seder DB, Dziodzio J, Smith KA, Hickey P, Bolduc B, Stone P, et al. Feasibility of bispectral index monitoring to guide early post-resuscitation cardiac arrest triage. *Resuscitation*. 2014;85(8):1030-6.
15. Stammet P, Collignon O, Werer C, Sertznig C, Devaux Y. Bispectral index to predict neurological outcome early after cardiac arrest. *Resuscitation*. 2014;85(12):1674-80.
16. Meex I, Dens J, Jans F, Boer W, Vanhengel K, Vundelinckx G, et al. Cerebral tissue oxygen saturation during therapeutic hypothermia in post-cardiac arrest patients. *Resuscitation*. 2013;84(6):788-93.
17. Genbrugge C, Eertmans W, Meex I, Van Kerrebroeck M, Daems N, Creemers A, et al. What is the value of regional cerebral saturation in post-cardiac arrest patients? A prospective observational study. *Crit Care*. 2016;20(1):327.
18. Nolan JP, Soar J, Cariou A, Cronberg T, Moulaert VR, Deakin CD, et al. European Resuscitation Council and European Society of Intensive Care Medicine Guidelines for Post-resuscitation Care 2015: Section 5 of the European Resuscitation Council Guidelines for Resuscitation 2015. *Resuscitation*. 2015;95:202-22.
19. Rundgren M, Rosen I, Friberg H. Amplitude-integrated EEG (aEEG) predicts outcome after cardiac arrest and induced hypothermia. *Intensive Care Med*. 2006;32(6):836-42.
20. Rundgren M, Westhall E, Cronberg T, Rosen I, Friberg H. Continuous amplitude-integrated electroencephalogram predicts outcome in hypothermia-treated cardiac arrest patients. *Crit Care Med*. 2010;38(9):1838-44.




21. Grenvik A, Safar P. Brain failure and resuscitation. New York: Churchill Livingstone; 1981. x, 268 p. p.
22. Claassen J, Taccone FS, Horn P, Holtkamp M, Stocchetti N, Oddo M, et al. Recommendations on the use of EEG monitoring in critically ill patients: consensus statement from the neurointensive care section of the ESICM. *Intensive Care Med.* 2013;39(8):1337-51.
23. Friberg H, Westhall E, Rosen I, Rundgren M, Nielsen N, Cronberg T. Clinical review: Continuous and simplified electroencephalography to monitor brain recovery after cardiac arrest. *Crit Care.* 2013;17(4):233.
24. Friedman D, Claassen J, Hirsch LJ. Continuous electroencephalogram monitoring in the intensive care unit. *Anesth Analg.* 2009;109(2):506-23.
25. Crepeau AZ, Fugate JE, Mandrekar J, White RD, Wijdicks EF, Rabinstein AA, et al. Value analysis of continuous EEG in patients during therapeutic hypothermia after cardiac arrest. *Resuscitation.* 2014;85(6):785-9.
26. Eertmans W, Genbrugge C, Haesevoets G, Dens J, Boer W, Jans F, et al. Recorded time periods of bispectral index values equal to zero predict neurological outcome after out-of-hospital cardiac arrest. *Crit Care.* 2017;21(1):221.
27. Fernandez-Torre JL, Hernandez-Hernandez MA. Utility of bilateral Bispectral index (BIS) monitoring in a comatose patient with focal nonconvulsive status epilepticus. *Seizure.* 2012;21(1):61-4.

28. Dahaba AA, Liu DW, Metzler H. Bispectral index (BIS) monitoring of acute encephalitis with refractory, repetitive partial seizures (AERRPS). *Minerva Anesthesiol.* 2010;76(4):298-301.
29. Chamorro C, Romera MA, Balandin B, Valdivia M. Nonconvulsive status and bispectral index. *Crit Care Med.* 2008;36(7):2218-9.
30. Ochiai K, Shiraishi A, Otomo Y, Koido Y, Kanemura T, Honma M. Increasing or fluctuating bispectral index values during post-resuscitation targeted temperature management can predict clinical seizures after rewarming. *Resuscitation.* 2017;114:106-12.
31. Karakis I, Montouris GD, Otis JA, Douglass LM, Jonas R, Velez-Ruiz N, et al. A quick and reliable EEG montage for the detection of seizures in the critical care setting. *J Clin Neurophysiol.* 2010;27(2):100-5.
32. Kolls BJ, Husain AM. Assessment of hairline EEG as a screening tool for nonconvulsive status epilepticus. *Epilepsia.* 2007;48(5):959-65.
33. Young GB, Sharpe MD, Savard M, Al Thenayan E, Norton L, Davies-Schinkel C. Seizure detection with a commercially available bedside EEG monitor and the subhairline montage. *Neurocrit Care.* 2009;11(3):411-6.
34. You KM, Suh GJ, Kwon WY, Kim KS, Ko SB, Park MJ, et al. Epileptiform discharge detection with the 4-channel frontal electroencephalography during post-resuscitation care. *Resuscitation.* 2017;117:8-13.


35. Westhall E, Rossetti AO, van Rootselaar AF, Wesenberg Kjaer T, Horn J, Ullen S, et al. Standardized EEG interpretation accurately predicts prognosis after cardiac arrest. *Neurology*. 2016;86(16):1482-90.
36. Hofmeijer J, Beernink TM, Bosch FH, Beishuizen A, Tjepkema-Cloostermans MC, van Putten MJ. Early EEG contributes to multimodal outcome prediction of postanoxic coma. *Neurology*. 2015;85(2):137-43.
37. Sivaraju A, Gilmore EJ, Wira CR, Stevens A, Rampal N, Moeller JJ, et al. Prognostication of post-cardiac arrest coma: early clinical and electroencephalographic predictors of outcome. *Intensive Care Med*. 2015;41(7):1264-72.
38. Stammet P, Wagner DR, Gilson G, Devaux Y. Modeling serum level of s100beta and bispectral index to predict outcome after cardiac arrest. *J Am Coll Cardiol*. 2013;62(9):851-8.

## Figure legends


**Fig 1. BIS VISTA™ monitor with EEG display.** The BIS VISTA™ device is able to display bilateral frontotemporal EEG traces in real-time.

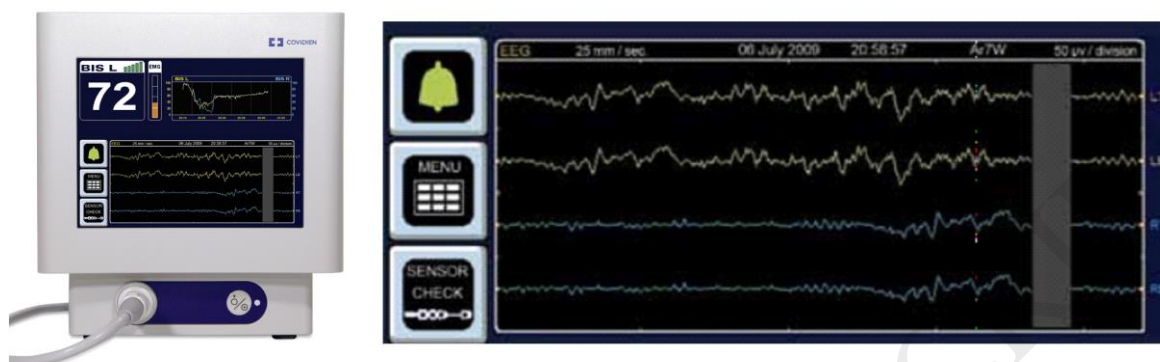

**Fig 2. Four typical electro-encephalic patterns after cardiac arrest.** These patterns are read-outs from raw simplified frontotemporal EEG traces which can be observed on the BIS monitor.

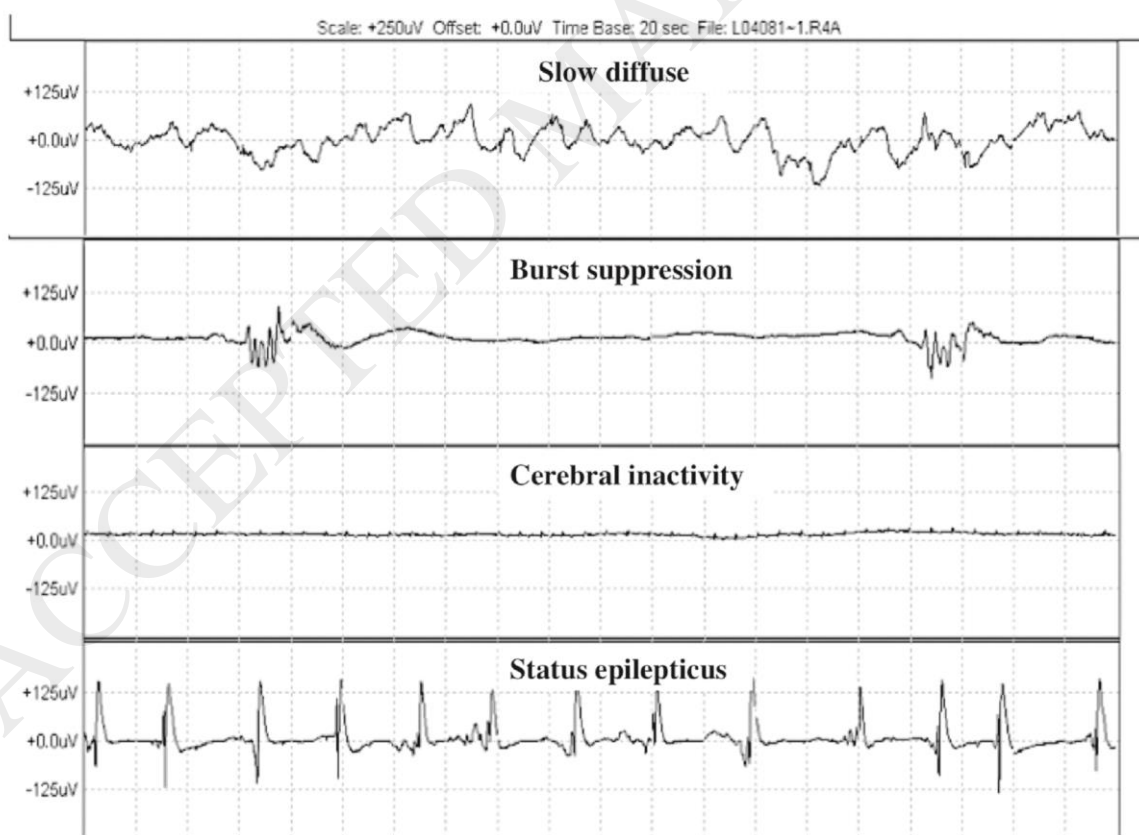

**Fig 3. Flowchart of enrolled patients.** BIS = Bispectral index; CA = cardiac arrest; CPC = Cerebral Performance Category; EEG = electro-encephalography.

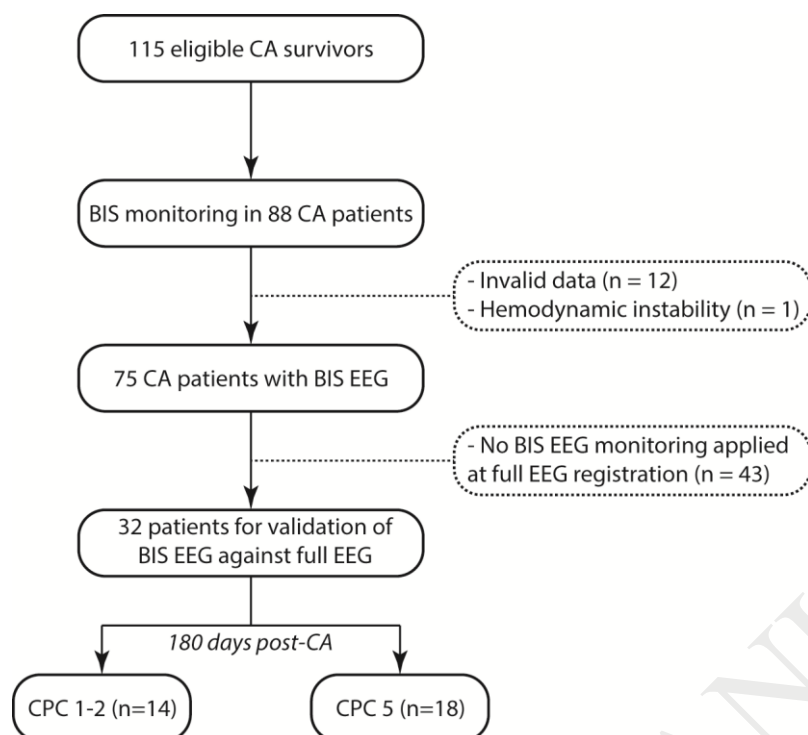

## Tables

**Table 1. Patient characteristics**

	All subjects	Good outcome CPC1-2	Poor outcome CPC3-5	P-value
Subjects, n (%)	32 (100)	14 (44)	18 (56)	
Age	61 ± 14	61 ± 14	61 ± 14	0.796
Male sex, n (%)	23 (72)	10 (71)	13 (72)	0.960
Initial rhythm				
Ventricular arrhythmia, n (%)	24 (75)	12 (86)	12 (67)	0.217
Witnessed arrest, n (%)	27 (84)	13 (93)	14 (78)	0.069
Time to ROSC, minutes	32 ± 20	24 ± 23	39 ± 13	<b>0.045</b>
CCU stay, days	10 ± 5	10 ± 5	9 ± 8	0.639
SE, n (%)	12 (38)	0 (0)	12 (67)	<b>&lt;0.001</b>
Time of validation, in days after cardiac arrest	3 ± 1	2 ± 1	3 ± 2	0.613
Number of full EEGs	3 ± 1	3 ± 1	3 ± 2	0.866

CPC: cerebral performance score – ROSC: return to spontaneous circulation – CCU: coronary care unit – SE: status epilepticus – EEG: electro-encephalogram.

Table 2. Validation of simplified BIS EEG

EEG patterns	Full EEG	Simplified BIS EEG		
		Neurophys. I	Neurophys. II	Consensus
<i>Slow diffuse (n)</i>	11	10	11	11
<i>Burst suppression (n)</i>	6	6	4	6
<i>Cerebral inactivity (n)</i>	3	3	3	3
<i>PEDs (n)</i>	4	1	1	1
<i>Status epilepticus (n)</i>	8	8	7	8
<b>Total</b>	32	28	26	29
<b>STATISTICS</b>				
<b>Sensitivity (%)</b>		86	71	86
<b>Specificity (%)</b>		91	100	100

EEG: Electroencephalogram – BIS: Bispectral index – PEDs: Periodic epileptic discharges.